


## **LASER EMITTER DVS-L-1010BAI**



A common breakdown of the handle is that the impulses do not pass, the patient does not feel tingling. Damage can be detected visually through the transparent part of the handle.

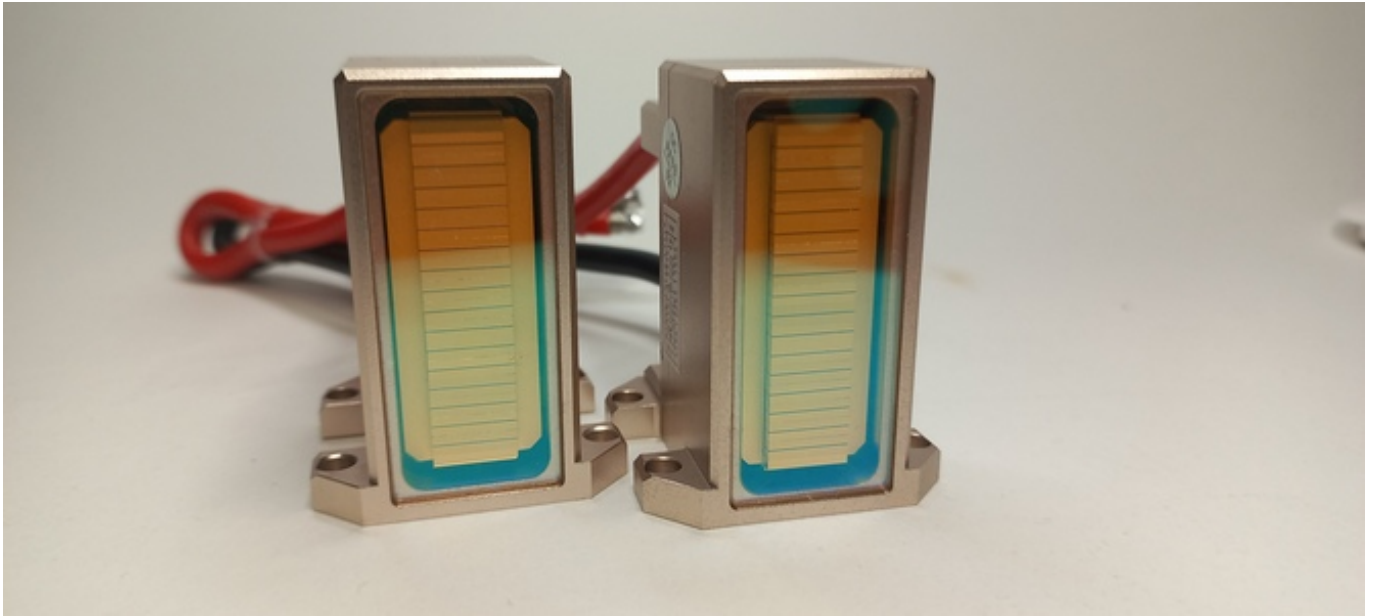

site [WWW.ROMSHI.COM](http://WWW.ROMSHI.COM)

Get your laser fixed - scan the QR to reach [www.romshi.com](http://www.romshi.com) and learn more about diode problems.